

Please type a plus sign (+) inside this box → ☒

PTO/SB/05 (12/97)  
Approved for use through 09/30/00. OMB 0651-0032  
Patent and Trademark Office: U.S. DEPARTMENT OF COMMERCE  
Under the Paperwork Reduction Act of 1995, no persons are required to respond to a collection of information unless it displays a valid OMB control number.

# UTILITY PATENT APPLICATION TRANSMITTAL

(Only for new nonprovisional applications under 37 CFR 1.53(b))

Attorney Docket No.	SELF-P-005-2	Total Pages	42
First Named Inventor or Application Identifier			
Jerome F. McAleer			
Express Mail Label No.	EM077162795US		

## APPLICATION ELEMENTS

See MPEP chapter 600 concerning utility patent application contents.

1. ☐ Fee Transmittal Form  
(Submit an original, and a duplicate for fee processing)
2. ☒ Specification [Total Pages 26]  
(preferred arrangement set forth below)
  - Descriptive title of the invention
  - Cross References to Related Applications
  - Statement Regarding Fed sponsored R & D
  - Reference to Microfiche Appendix
  - Background of the Invention
  - Brief Summary of the Invention
  - Brief Description of the Drawings (if filed)
  - Detailed Description
  - Claim(s)
  - Abstract of the Disclosure
3. ☒ Drawing(s) (35 USC 113) [Total Sheets 8]
4. Oath or Declaration [Total Pages 4]
  - a. ☐ Newly executed (original or copy)
  - b. ☒ Copy from a prior application (37 CFR 1.63(d))  
(for continuation/divisional with Box 17 completed)  
(Note Box 5 below)
    - i. ☐ DELETION OF INVENTOR(S)  
Signed statement attached deleting inventor(s) named in the prior application, see 37 CFR 1.63(d)(2) and 1.33(b).
5. ☒ Incorporation By Reference (useable if Box 4b is checked)  
The entire disclosure of the prior application, from which a copy of the oath or declaration is supplied under Box 4b, is considered as being part of the disclosure of the accompanying application and is hereby incorporated by reference therein.

ADDRESS TO: Assistant Commissioner for Patents  
Box Patent Application  
Washington, DC 20231

6. ☐ Microfiche Computer Program (Appendix)
7. Nucleotide and/or Amino Acid Sequence Submission (if applicable, all necessary)
  - a. ☐ Computer Readable Copy
  - b. ☐ Paper Copy (identical to computer copy)
  - c. ☐ Statement verifying identity of above copies

## ACCOMPANYING APPLICATION PARTS

8. ☐ Assignment Papers (cover sheet & document(s))
9. ☐ 37 CFR 3.73(b) Statement (when there is an assignee) ☐ Power of Attorney
10. ☐ English Translation Document (if applicable)
11. ☐ Information Disclosure Statement (IDS)/PTO-1449 ☐ Copies of IDS Citations
12. ☒ Preliminary Amendment
13. ☒ Return Receipt Postcard (MPEP 503)  
(Should be specifically itemized)
14. ☐ Small Entity ☐ Statement filed in prior application, Status still proper and desired
15. ☐ Certified Copy of Priority Document(s) (if foreign priority is claimed)
16. ☒ Other: exp mail cert

17. If a CONTINUING APPLICATION, check appropriate box and supply the requisite information:

☒ Continuation ☐ Divisional ☐ Continuation-in-part (CIP) of prior application No: 08 / 601,223

## 18. CORRESPONDENCE ADDRESS

☐ Customer Number or Bar Code Label

(Insert Custom)



or ☐ Correspondence address below

NAME

21121

ADDRESS

CITY

STATE

ZIP CODE

COUNTRY

TELEPHONE

FAX

Burden Hour Statement: This form is estimated to take 0.2 hours to complete. Time will vary depending upon the needs of the individual case. Any comments on the amount of time you are required to complete this form should be sent to the Chief Information Officer, Patent and Trademark Office, Washington, DC 20231. DO NOT SEND FEES OR COMPLETED FORMS TO THIS ADDRESS. SEND TO: Assistant Commissioner for Patents, Box Patent Application, Washington, DC 20231.

IN THE UNITED STATES PATENT AND TRADEMARK OFFICE

CERTIFICATE OF MAILING UNDER 37 C.F.R. 1.10


Applicants : McAleer et al.  
Serial No. : to be assigned  
Filing Date : herewith  
Title of Invention : Disposable Glucose Test Strips, and  
Methods and Compositions for Making  
Same  
Title of Papers : Application; Transmittal Letter

"Express Mail" Mailing Label  
Number EM077162795US

Date of Deposit January 12, 1998

I hereby certify that these papers and fee are  
being deposited with the United States Postal Service  
"Express Mail Post Office to Addressee" service under 37  
C.F.R. 1.10 on the date indicated above and is addressed  
to the Commissioner of Patents and Trademarks,  
Washington, D.C. 20231.

Marina T. Larson  
(Typed or Printed Name of Person  
mailing paper or fee)

  
(Signature of Person mailing  
paper or fee)

IN THE UNITED STATES PATENT AND TRADEMARK OFFICE

Applicants: McAleer et al.

Serial No.: to be assigned

Examiner:

Filed: herewith

Art Unit:

For: DISPOSABLE GLUCOSE TEST STRIPS AND METHOD AND  
COMPOSITION FOR MAKING SAME

PRELIMINARY AMENDMENT

Asst. Commissioner for Patents  
Washington, D.C. 20231

Sir:

Preliminary to the examination of the continuation application which is filed  
herewith, please make the following amendments:

In the specification:

Page 1, before line 1, insert

--This application is a continuation of US Patent Application No. 08/601,223,  
issued January 13, 1998 as US Patent No. 5,708,247, which is incorporated herein by reference.--

In the claims:

Please cancel claims 1-16 and 19-35.

REMARKS

This amendment to made to include a reference to the parent application, and to cancel claims of overlapping scope with the parent. No new matter has been added.

Respectfully submitted,



Marina T. Larson

PTO Reg. No. 32,038

Attorney for Applicant  
(914) 245-3252

OPPEDAHL & LARSON  
1992 COMMERCE STREET, SUITE 309  
YORKTOWN HEIGHTS, NY 10598

---

TO ALL WHOM IT MAY CONCERN:

Be it known that we, Jerome F. McAleer, David Scott, Geoff Hall, Manuel Icaza-Alvarez and Elliot V. Plotkin, have invented an improvement in

DISPOSABLE GLUCOSE TEST STRIPS, AND METHODS  
AND COMPOSITIONS FOR MAKING SAME

of which the following is a

SPECIFICATION

BACKGROUND OF THE INVENTION

This application relates to disposable glucose test strips for use in electrochemical determinations of blood glucose, and to methods and compositions for use in making such strips.

Glucose monitoring is a fact of everyday life for diabetic individuals, and the accuracy of such monitoring can literally mean the difference between life and death. To accommodate a normal life style to the need for frequent monitoring of glucose levels, a number of glucose meters are now available which permit the individual to test the glucose level in a small amount of blood.

Many of these meters detect glucose in a blood sample electrochemically, by detecting the oxidation of blood glucose using an enzyme such as glucose oxidase provided as part of a disposable, single use electrode system. Examples of devices of this type are disclosed in European Patent No. 0 127 958, and US Patents Nos. 5,141,868, 5,286,362, 5,288,636, and 5,437,999 which are incorporated herein by reference.

In general, existing glucose test strips for use in electrochemical meters comprise a substrate, working and reference electrodes formed on the surface of the substrate, and a means for making connection between the electrodes and the meter. The working electrode is coated with an enzyme capable of oxidizing glucose, and a mediator compound which transfers electrons from the enzyme to the electrode resulting in a measurable current when glucose is present. Representative mediator compounds include ferricyanide, metallocene compounds such as ferrocene, quinones, phenazinium salts, redox indicator DCPIP, and imidazole-substituted osmium compounds.

Working electrodes of this type have been formulated in a number of ways. For example, mixtures of conductive carbon, glucose oxidase and a mediator have been formulated into a paste or ink and applied to a substrate. EP 0 127 958 and US 5,286,362. In the case of disposable

glucose strips, this application is done by screen printing in order to obtain the thin layers suitable for a small flat test strip. The use of screen printing, however, introduces problems to the operation of the electrode.

5                   Unlike a thicker carbon paste electrode which remains fairly intact during the measurement, screen printed electrodes formed from carbon pastes or inks are prone to break up on contact with the sample. The consequences of this breakup are two-fold. Firstly, the components of the electrode formulation are released into solution. Once 10 these components drift more than a diffusion length away from the underlying conductive layer, they no longer contribute toward the measurement, but in fact diminish the response by depleting inwardly-diffusing analyte. Secondly, the breakup of the screen printed electrode means that the effective electrode area is falling over time. 15

20                   The combination of these two effects results in current transients which fall rapidly from an initial peak over the period of the measurement, and a high sensitivity to oxygen which quickly competes with the mediator for the enzyme. This fact is clearly demonstrated by the much lower currents measured in blood samples than in plasma samples or other aqueous media, and can result in erroneous readings. A further consequence is that the transients are often 25 "lumpy" as the electrode breaks up in a chaotic manner.

Lumpy transients either give rise to erroneous readings or rejected strips, neither of which are acceptable.

5 In addition to the potential for electrode breakup of screen-printed carbon-based electrodes, known electrodes used in disposable glucose test strips have been kinetically-controlled, i.e., the current depends on the rate of conversion of glucose by the enzyme. Because the response measured by the instrument represents a balance between the reaction of enzyme and mediator, enzyme and glucose and enzyme and oxygen, and because each of these reactions has its own dependence on temperature, the response of a kinetically-controlled test strip is very sensitive to the temperature of the sample. Substantial variation in the measured glucose value can therefore occur as a result of variations in sample handling.

10 Because of the importance of obtaining accurate glucose readings to the well-being of a patient using the meter and disposable test strips, it would be highly desirable to have a glucose test strip which did not suffer from these drawbacks, and which therefore provided a more consistent and reliable indication of actual blood glucose values, regardless of actual conditions. It is therefore an object of the present invention to provide disposable glucose test strips which are not prone to electrode breakup on contact with a sample.



It is a further object of this invention to provide glucose test strips which provide a glucose reading that is essentially independent of the hematocrit of the sample.

5 It is a further object of the present invention to provide glucose test strips which are substantially independent of temperature over a range between normal body temperature and room temperature.

10 It is a further object of the invention to provide test strips which provide a substantially flat current transient, without significant decay for periods of at least 10 seconds after the peak current level is obtained.

#### SUMMARY OF THE INVENTION

15 The present invention provides an improved disposable glucose test strip for use in a test meter of the type which receives a disposable test strip and a sample of blood from a patient and performs an electrochemical analysis of the amount of glucose in the sample. The test  
20 strip comprises:

- (a) a substrate;
  - (b) a reference electrode;
  - (c) a working electrode; and
  - (d) means for making an electrical connection
- 25 between the reference and working electrode and a glucose

test meter. The working electrode comprises a conductive base layer disposed on the substrate and a non-conductive coating disposed over the conductive base layer. The non-conductive coating comprises a filler which has both hydrophobic and hydrophilic surface regions, an enzyme effective to oxidize glucose, e.g., glucose oxidase, and a mediator effective to transfer electrons from the enzyme to the conductive base layer. The filler is selected to have a balance of hydrophobicity and hydrophilicity such that on drying it forms a two-dimensional network on the surface of the conductive base layer. Preferred filler are non-conductive silica fillers. The response of this test strip is dependent on the diffusion rate of glucose, not on the rate at which the enzyme can oxidize glucose, such that the performance of the test strip is essentially temperature independent over relevant temperature ranges. Further, the silica appears to form a two-dimensional network which excludes red blood cells, thus rendering the test strip substantially insensitive to the hematocrit of the patient.

#### BRIEF DESCRIPTION OF THE DRAWINGS

Figs. 1A and 1B shows an electrode structure useful in a disposable test strip in accordance with the invention;

Fig. 2 shows a test strip in accordance with the invention;

Figs. 3A - 3C show the current measured as a function of glucose concentration for three different hematocrit levels;

Fig. 4 shows the relationship of the glucose-concentration dependence of the measured current as a function of hematocrit;

Figs. 5A - 5C show the current measured as a function of glucose in blood and a control solution for three different variations of the conductive base layer;

Fig. 6A and 6B show the current measured as a function of glucose at two different temperatures;

Fig. 7 shows a further embodiment of a glucose test strip according to the invention; and

Figs 8A and 8B show a current transients observed using a test strip according to the invention and a commercial carbon-based test strip.

#### DETAILED DESCRIPTION OF THE INVENTION

Figs. 1A and 1B show electrodes useful in a disposable test strip in accordance with the invention. As shown, the electrodes are formed on a substrate 10. On the substrate 10 are placed a conductive base layer 16, a working electrode track 14, a reference electrode track 15,

and conductive contacts 11, 12, and 13. An insulating mask 18 is then formed, leaving a portion of the conductive base layer 16, and the contacts 11, 12 and 13 exposed. A region of a working coating 17 is then applied over the insulating mask 18 to make contact with conductive base layer 16.

The assembly shown in Fig. 1 provides a fully functional assembly for the measurement of blood glucose when connected to a meter. Advantageously, however, the electrode strips of the invention are finished by applying a polyester mesh 21 over the region of the working coating 17 of the electrode assembly 22, and then a top cover 23 to prevent splashing of the blood sample. (Fig. 2) The polyester mesh acts to guide the sample to the reference electrode, thereby triggering the device and initiating the test.

The substrate 10 used in making the test strips of the invention can be any non-conducting, dimensionally stable material suitable for insertion into a glucose test meter. Suitable materials include polyester films, for example a 330 micron polyester film, and other insulating substrate materials.

The working electrode track 15, the reference electrode track 14, and conductive contacts 11, and 12 can be formed from essentially any conductive material including silver, Ag/AgCl, gold, or platinum/carbon.

5 The conductive base layer 16 is preferably formed from conductive carbon. Preferred conductive carbon are ERCON ERC1, ERCON ERC2 and Acheson Carbon Electrode 423. Carbon with these specifications is available from Ercon Inc. (Waltham, Massachusetts, USA), or Acheson Colloids, (Princes Rock, Plymouth, England). The conductive base layer 16 makes contact with working electrode track 15, and is close too but not contacting the end of reference electrode track 15.

10 The insulating layer 18 can be formed from polyester-based printable dielectric materials such as ERCON R488-B(HV) -B2 Blue.

15 The key to the performance achieved using the present invention is in the nature of the coating 17. This coating contains a filler which has both hydrophobic and hydrophilic surface regions, an enzyme which can oxidize glucose, and a mediator which can transfer electrons from the enzyme to the underlying conductive base layer 16.

20 A preferred filler for use in the coating 17 is silica. Silica is available in a variety of grades and with a variety of surface modifications. While all silica compounds tested resulted in a product which could measure glucose under some conditions, the superior performance characteristics of glucose test strip of the invention are  
25 obtained when a silica having a surface modification to

render it partially hydrophobic is used. Materials of this type include Cab-O-Sil TS610, a silica which is modified by partial surface treatment with methyl dichlorosilane; Cab-o-Sil 530, a silica which is modified by full surface treatment with hexamethyl disilazane; Spherisorb C4 silica, which is surface modified with 4 carbon chains; and other similarly modified by silicas, or combinations thereof. Silica with a surface modification which is too hydrophobic should be avoided, however, since it has been observed that C18-modified silica is too hydrophobic to form a printable ink.

During the process of manufacturing the ink of the invention, the particles are broken down by homogenization to expose hydrophilic inner portions of the silica particles. The actual particles present in the ink therefore have both hydrophilic and hydrophobic regions. The hydrophilic regions form hydrogen bonds with each other and with water.

When this material is formulated into an ink as described below in Example 1, and screen printed onto the conductive base layer 16, the dual nature of the material causes it to form layers of two-dimensional networks which take form as a kind of honeycomb. On rehydration, this layer does not break up, but swells forming a gelled reaction zone in the vicinity of the underlying conductive

base layer 16. Enzyme, mediator and glucose move freely within this zone, but interfering species such as red blood cells containing oxygenated hemoglobin are excluded. This results in a device which the amount of current generated in response to a given amount of glucose varies by less than 10 percent over a hematocrit range of 40 to 60 %, and which is thus substantially insensitive to the hematocrit of the sample, and in fact performs substantially the same in blood as in a cell-free control solution. (Figs. 3A-C, Fig. 4 and Fig. 5A - 5C)

Furthermore, the gelled reaction zone presents a greater barrier to entry of glucose which makes the device diffusion, rather than kinetically limited. This leads to a device in which the measured current varies by less than 10 percent over a temperature range from 20°C to 37°C and which is thus essentially temperature independent. (Figs. 6A and 6B)

The working layer is advantageously formed from an aqueous composition containing 2 to 10 % by weight, preferably 4 to 10 % and more preferably about 4.5 % of a binder such as hydroxyethylcellulose or mixtures of hydroxyethylcellulose with alginate or other thickeners; 3 to 10 % by weight, preferably 3 to 5 % and more preferably about 4 % silica; 8 to 20 % by weight, preferably 14 to 18 % and more preferably about 16 % of a mediator such as

ferricyanide; and .4 to 2 % by weight, preferably 1 to 2 % and more preferably about 1.6 % of an enzyme such as glucose oxidase, assuming a specific activity of about 250 units/mg, or about 1000 to 5000 units per gram of ink formulation.

5           The working layer may also include additional ingredients without departing from the scope of the invention. For example, the nonconducting layer may include an antifoam. In addition, the nonconducting layer may be formulated with a buffering agent to control the pH of the reaction zone. The pH may be maintained at a level within the range from about pH 3 to pH 10. It is of particular utility to maintain the pH of the device at a level above 8 because at this pH oxygen bound to hemoglobin is not released. Further, at this pH, the reaction rate of glucose oxidase with oxygen is very low. Thus, selection of an  
10           appropriate pH can further stabilize the performance of the test strip against the effects of varying hematocrit.

15           Fig. 7 shows an alternative embodiment of the invention. In this embodiment, a second working layer 71 is disposed over the first working layer 17. This layer is formed from a composition which is identical to the first working layer except that the enzyme or both the enzyme and the mediator are omitted. This layer further isolates the conductive base layer from contact with oxygen-carrying red  
20           blood cells, thus reducing the effects of oxygen.



Furthermore, to the extent that enzyme may tend to diffuse away from the surface of the electrode during the course of the measurement, this layer provides an increased region in which it will have mediator available for the transfer of electrons.

EXAMPLE 1

A non-conducting formulation for preparation of the working layer 17 was made as follows. 100 ml of 20 mM aqueous trisodium citrate was adjusted to pH 6 by the addition of 0.1 M citric acid. To this 6 g of hydroxyethyl cellulose (HEC) was added and mixed by homogenization. The mixture was allowed to stand overnight to allow air bubbles to disperse and then used as a stock solution for the formulation of the coating composition.

2 grams Cab-o-Sil TS610 silica and 0.1 grams of Dow Corning antifoam compound was gradually added by hand to 50 grams of the HEC solution until about 4/5 ths of the total amount has been added. The remainder is added with mixing by homogenization. The mixture is then cooled for ten minutes in a refrigerator. 8 g of potassium hexacyanoferrate (III) is then added and mixed until completely dissolved. Finally, 0.8 g of glucose oxidase enzyme preparation (250 Units/mg) is added and the thoroughly mixed into the solution. The resulting

formulation is ready for printing, or can be stored with refrigeration.

EXAMPLE 2

5 To prepare glucose test strips using the ink formulation of Example 1, a series of patterns are used to screen print layers onto a 330 micron polyester substrate (Melinex 329). The first step is the printing of carbon pads. An array of 10 X 50 pads of carbon is formed on the surface of the polyester substrate by printing with EC2 carbon. (Ercon) The printed substrate is then passed through a heat ed dryer, and optionally cured at elevated temperature (e.g. 70°C) for a period of 1 to 3 weeks.

10 Next, an array of silver/silver chloride connecting tracks and contacts is printed onto the substrate using ERCON R-414 (DPM-68)1.25 bioelectrode sensor coating material and dried. One working track which makes contact with the carbon pad and one reference track is printed for each carbon pad in the array.

15 A dielectric layer is then printed using ERCON R488-B(HV) -B2 Blue and dried. The dielectric layer is printed in a pattern which covers substantially all of each devices, leaving only the contacts, the tip of the reference electrode and the carbon pads uncovered.

On top of the dielectric layer the ink of Example 1 is used to form a working layer overlaid on top of each conductive carbon pad.

5 Polyester mesh strips (Scrynel PET230 HC) are then laid down across the substrate in lines, covering the reactions areas exposed by the windows in the dielectric. An 5 mm wide polyester strip (50 microns thick) is then applied over the top of the mesh strips, and the edges of the electrodes are heat sealed. Finally, the substrate is cut up to provide 50 individual electrodes, for example having a size of 5.5 mm wide and 30 mm long.

### EXAMPLE 3

15 Test strips manufactured using the ink formulation of Example 1 in the manner described in Example 2 were placed in a test meter with an applied voltage of 500 mV and used to test blood samples having varying glucose concentrations and hematocrits ranging from 40% to 60%. Figs. 3A-3C show the current measured 25 seconds after applying the voltage as a function of the glucose concentration, and Fig. 4 plots the slope of the glucose response as a function of hematocrit. As can be seen, the indicators produce highly reproducible current levels which are essentially independent of hematocrit.

EXAMPLE 4

Glucose test strips in accordance with the invention were made in accordance with Example 2, except the non-conductive layer was formed with 7 g Spherisorb C4 and 1 g Cab-o-Sil TS610. This formulation was laid down on two three different types of carbon-containing conductive base layers as follows:

A: Ercon EC1

B: Ercon EC2

C: Ercon EC2 on top of Acheson Carbon, Electrodag 423 SS.

These test strips were used to measure varying levels of glucose in either a control solution (One Touch Control Solution, Lifescan Inc.) containing glucose in an inert solution or in blood at an applied voltage of 425 mV. The current observed 25 seconds after the voltage was applied was measured. Figs. 5A - 5C show the results obtained for the three formulations, A, B, and C, respectively. In all cases, the slope of the line showing the response of the meter to different glucose concentrations was essentially the same whether the measurement were made in blood or the control solution. Thus, this further demonstrates the independence of the test strips of the invention from the oxygen content and hematocrit of the sample, as well as the

ability to use varied material as the conductive base layer.

EXAMPLE 5

Test strips prepared in accordance with Example 2 were tested at two different sample temperatures, namely 37 °C and 20 °C using an applied voltage of 425 mV. Figs. 6A and 6B show the current measured 25 seconds after applying the voltage as a function of glucose concentration. As can be seen, the slopes of the two lines are essentially identical (0.1068 at 20 °C versus 0.1009 at 37 °C), thus demonstrating that the test strips provide essentially temperature-independent behavior over a temperature range from ambient to physiological temperatures.

EXAMPLE 6

The current transient was measured for a test strip prepared in accordance with Example 2 and for a commercial test strip made with a carbon-containing ink. The results are shown in Figs. 8A and 8B. As shown, the test strip of the invention (Fig. 8A) provides a very flat transient which maintains more than 50% of the peak current for a period of more than 25 seconds after the initial response from the test strip. In contrast, the carbon-based electrode exhibited an almost immediate decay in the current, having lost 50% of the peak current in a period of

the first 1 to 2 seconds after the initial response from the test strip. This makes timing of the measurement difficult if peak current values are to be captured, or reduces the dynamic range of the meter if currents must be measured after substantial decay has occurred. Thus, the test strips of the invention are advantageous in that they provide test strips in which the amount of current generated in response to a given amount of glucose decays by less than 50% in the 5 seconds following peak current generation.

We Claim:

1                   1.    A disposable glucose test strip for use in a  
2    test meter of the type which receives a disposable test  
3    strip and a sample of blood from a patient and performs an  
4    electrochemical analysis of the amount of glucose in the  
5    sample, comprising:

6                   (a)   a substrate;

7                   (b)   a reference electrode;

8                   (c)   a working electrode, said working electrode  
9    comprising a conductive base layer disposed on the substrate  
10   and a first working coating disposed over the conductive  
11   base layer, said first working coating comprising a filler  
12   having both hydrophobic and hydrophilic surface regions such  
13   that it forms a network upon drying, an enzyme effective to  
14   oxidize glucose, and a mediator effective to transfer  
15   electrons from the enzyme to the conductive base layer; and

16                   (d)   means for making an electrical connection  
17   between the reference and working electrode and a glucose  
18   test meter.

1                   2.    The test strip of claim 1, wherein the  
2    working layer is non-conductive.

1                   3.    The test strip of claim 2, wherein the filler  
2    is silica.

1           4.    The test strip of claim 3, wherein the  
2   conductive base layer comprises conductive carbon.

1           5.    The test strip of claim 3, wherein the enzyme  
2   is glucose oxidase.

1           6.    The test strip according to claim 3, wherein  
2   the mediator is ferricyanide.

1           7.    The test strip of claim 3, wherein the first  
2   working layer is formed from an aqueous composition  
3   comprising weight 2 to 10 % by weight of a binder 3 to 10 %  
4   by weight of silica; 8 to 20 % by weight of a mediator; and  
5   1000 to 5000 units per gram of the aqueous composition of an  
6   enzyme for oxidizing glucose.

1           8.    The test strip of claim 3, wherein the silica  
2   is Cab-o-Sil TS610.

1           9.    The test strip of claim 8, wherein the  
2   conductive base layer comprises conductive carbon.

1           10.   The test strip of claim 8, wherein the enzyme  
2   is glucose oxidase.



1                   11. The test strip of claim 8, wherein the  
2 mediator is ferricyanide.

1                   12. The test strip of claim 8, wherein the first  
2 working layer is formed from an aqueous composition  
3 comprising weight 2 to 10 % by weight of a binder 3 to 10 %  
4 by weight of silica; 8 to 20 % by weight of a mediator; and  
5 1000 to 5000 units per gram of the aqueous composition of an  
6 enzyme for oxidizing glucose.

1                   13. The test strip of claim 3, further comprising  
2 a second working layer comprising silica, a binder and a  
3 mediator but no glucose-oxidizing enzyme.

1                   14. The test strip of claim 3, further comprising  
2 a second working layer comprising silica and a binder but no  
3 glucose-oxidizing enzyme.

1                   15. The test strip of claim 1, further comprising  
2 a second working layer comprising a filler, a binder and a  
3 mediator but no glucose-oxidizing enzyme.

1                   16. The test strip of claim 1, further comprising  
2 a second working layer comprising a filler and a binder but  
3 no glucose-oxidizing enzyme.

1                   17. An aqueous composition comprising a binder, a  
2 filler having both hydrophobic and hydrophilic surface  
3 regions, at least one of an enzyme effective to oxidize  
4 glucose and an electron transfer mediator.

1                   18. The composition of claim 17, wherein the  
2 filler is non-conductive.

1                   19. The composition of claim 18, wherein the  
2 filler is silica.

1                   20. An aqueous composition comprising 2 to 10 %  
2 by weight of a binder; 3 to 10 % by weight of silica; 8 to  
3 20 % by weight of a mediator; and 1000 to 5000 units per  
4 gram of the aqueous composition of an enzyme for oxidizing  
5 glucose.

1                   21. The composition of claim 20, wherein the  
2 silica both hydrophobic and hydrophilic surface regions.

1                   22. The composition of claim 21, wherein the  
2 binder is hydroxyethylcellulose.

1                   23. The composition of claim 20, wherein the  
2 enzyme is glucose oxidase.

1                   24. The composition of claim 20, wherein the  
2 mediator is ferricyanide.

1                   25. A method for making a disposable test strip  
2 for the electrochemical detection of glucose, comprising the  
3 steps of:

4                   (a) applying working and reference electrode  
5 tracks to a substrate;

6                   (b) applying a conductive base layer in contact  
7 with the working electrode track; and

8                   (c) applying a working layer over the conductive  
9 base layer, wherein the working layer comprising a filler  
10 having both hydrophobic and hydrophilic surface regions such  
11 that it forms a network upon drying, an enzyme effective to  
12 oxidize glucose, and a mediator effective to transfer  
13 electrons from the enzyme to the conductive base layer.

1                   26. The method of claim 25, wherein the filler is  
2 non-conductive.

1                   27. The method of claim 26, wherein the filler is  
2 silica.

1                   28. The method of claim 27, wherein the  
2                   conductive base layer comprises conductive carbon.

1                   29. The method of claim 27, wherein the enzyme is  
2                   glucose oxidase.

1                   30. The method of claim 27, wherein the mediator  
2                   is ferricyanide.

1                   31. The method of claim 27, wherein the first  
2                   working layer is formed from an aqueous composition  
3                   comprising weight 2 to 10 % by weight of a binder 3 to 10 %  
4                   by weight of silica; 8 to 20 % by weight of a mediator; and  
5                   1000 to 5000 units per gram of the aqueous composition of an  
6                   enzyme for oxidizing glucose.

1                   32. The method of claim 31, wherein the silica is  
2                   Cab-o-Sil TS610.

1                   33. A disposable glucose test strip which  
2                   produces a current indicative of the amount of glucose in a  
3                   sample applied to the strip in response to an applied  
4                   voltage, wherein the amount of current generated in response

5 to a given amount of glucose varies by less than 10 percent  
6 over a temperature range from 20°C to 37°C.

1 34. A disposable glucose test strip which  
2 produces a current indicative of the amount of glucose in a  
3 sample applied to the strip in response to an applied  
4 voltage, wherein the amount of current generated in response  
5 to a given amount of glucose varies by less than 10 percent  
6 over a hematocrit range of 0 to 60 %.

1 35. A disposable glucose test strip which  
2 produces a current indicative of the amount of glucose in a  
3 sample applied to the strip in response to an applied  
4 voltage, wherein the amount of current generated in response  
5 to a given amount of glucose decays by less than 50% in the  
6 5 seconds following peak current generation.

ABSTRACT OF THE DISCLOSURE

1           An improved disposable glucose test strip for use  
2           in a test meter of the type which receives a disposable test  
3           strip and a sample of blood from a patient and performs an  
4           electrochemical analysis is made using a working formulation  
5           containing a filler, an enzyme effective to oxidize glucose,  
6           e.g., glucose oxidase, and a mediator effective to transfer  
7           electrons from the enzyme. The working formulation is  
8           printed over a conductive carbon base layer to form a  
9           working electrode. The filler, for example a silica filler,  
10          is selected to have a balance of hydrophobicity and  
11          hydrophilicity such that one drying it forms a two-  
12          dimensional network on the surface of the conductive base  
13          layer. The response of this test strip is essentially  
14          temperature independent over relevant temperature ranges and  
15          is substantially insensitive to the hematocrit of the  
16          patient.

Fig. 1A

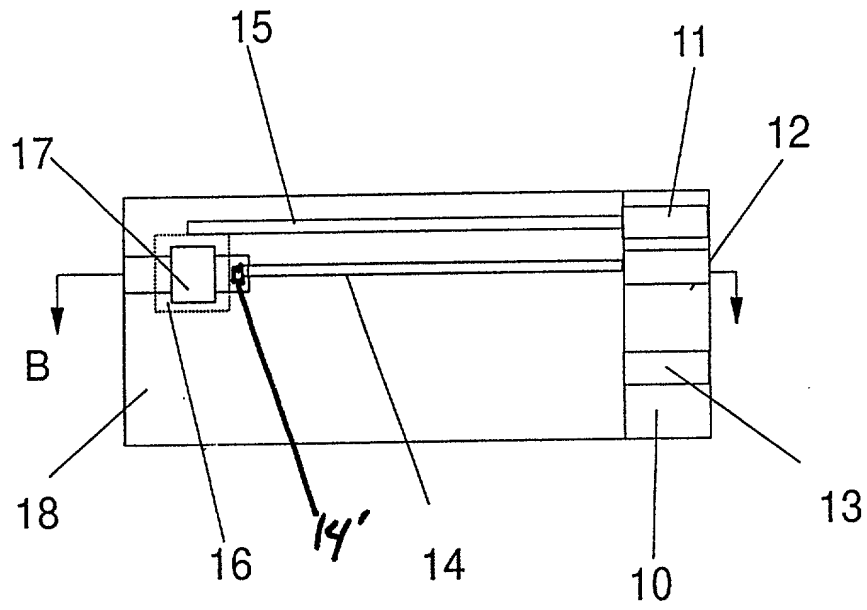
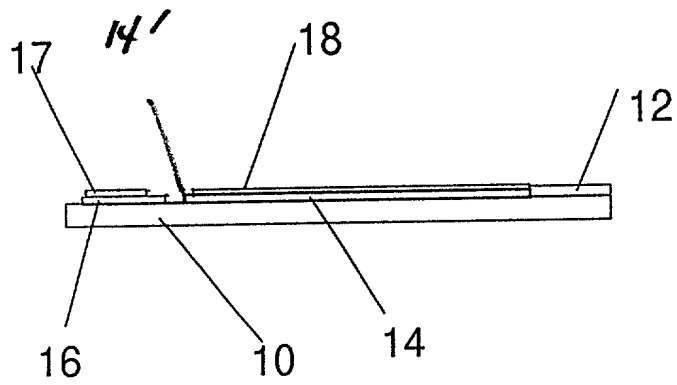


Fig. 1 B



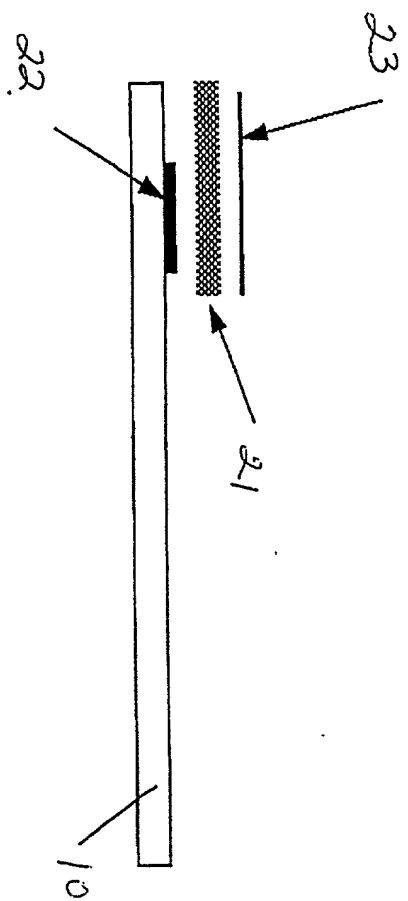


Fig 2



Fig. 3A 60 % Haematocrit, measured at 500 mV

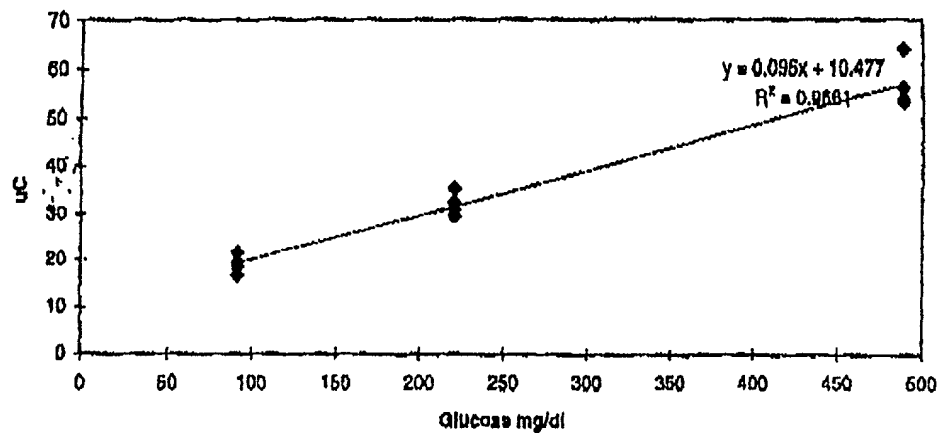


Fig. 3B 50% Haematocrit, measured at 500mV


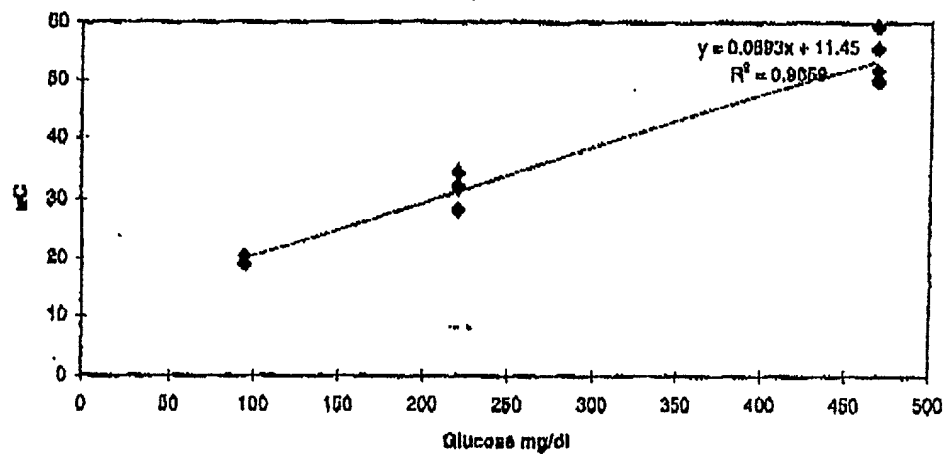


Fig. 3C 40% Haematocrit, measured at 500 mV

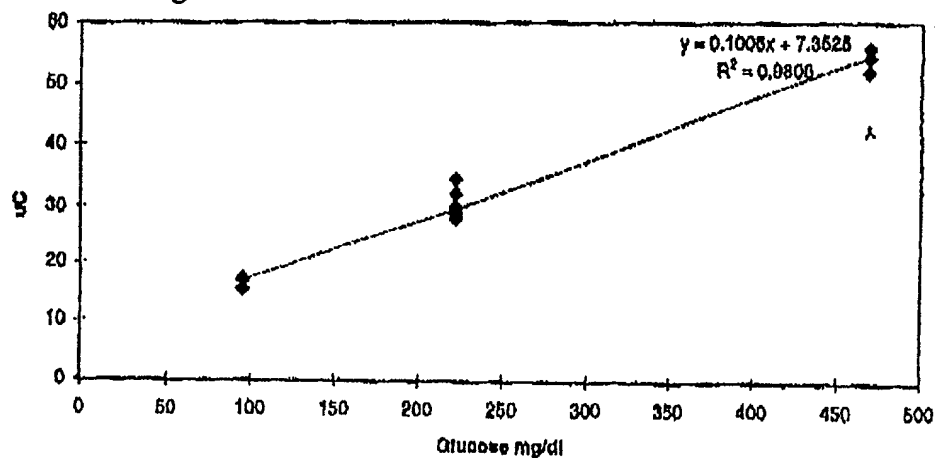

# Fig. 4

Glucose Response vs. Hematocrit

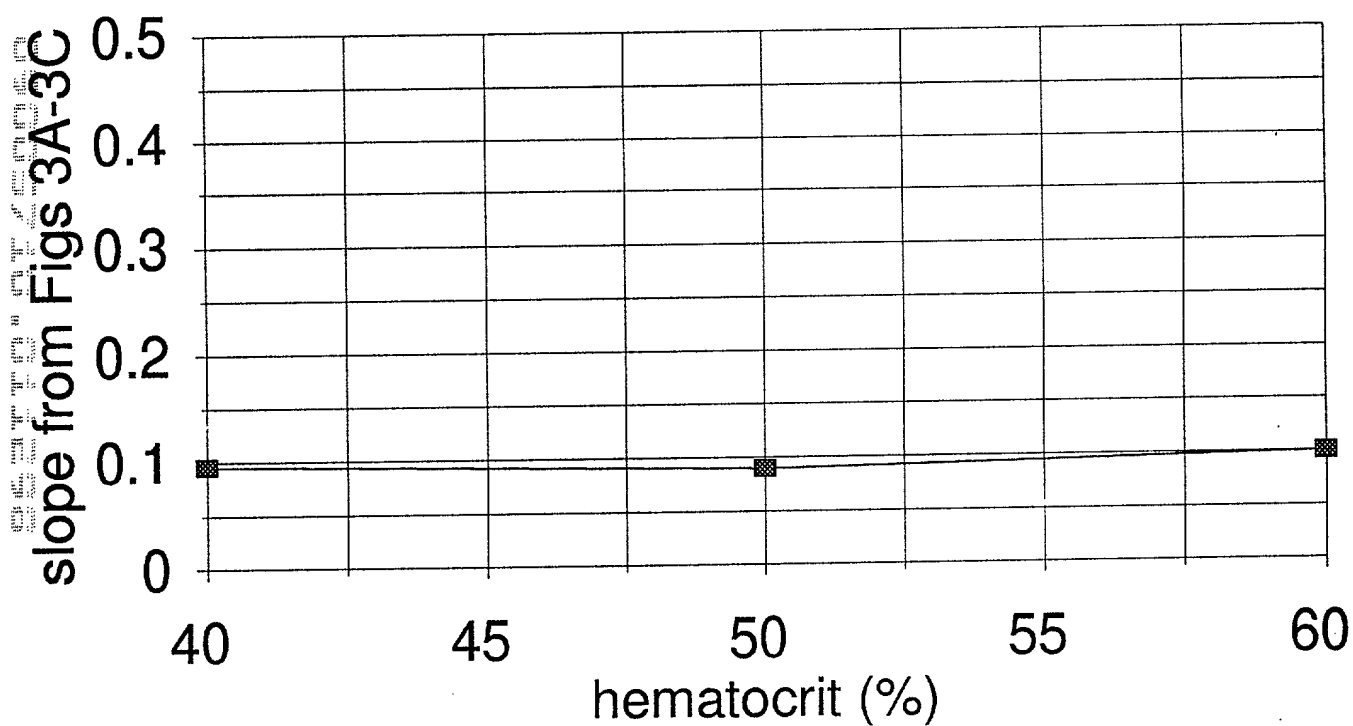


Fig. 5A

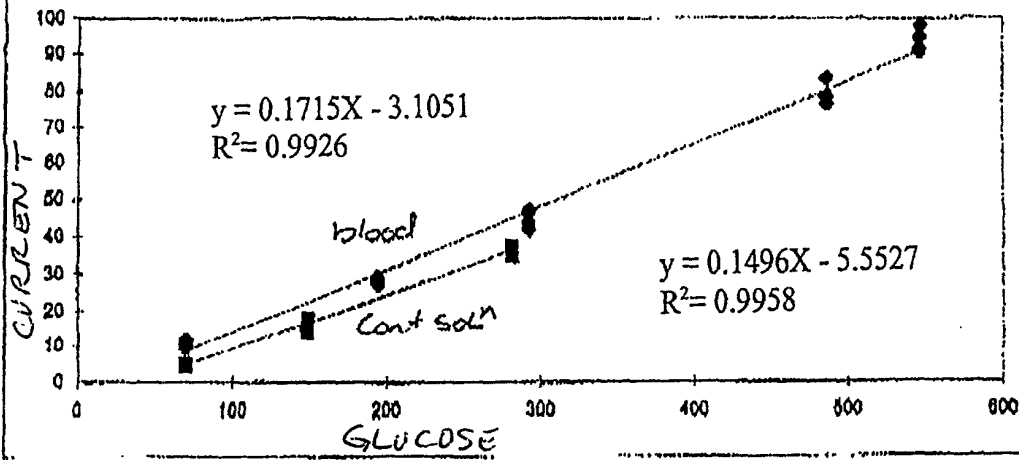


Fig. 5B

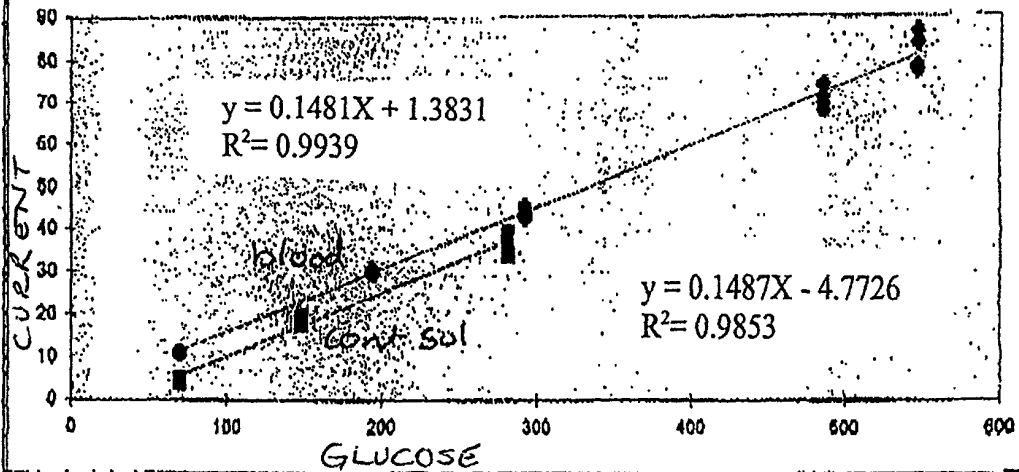


Fig. 5C

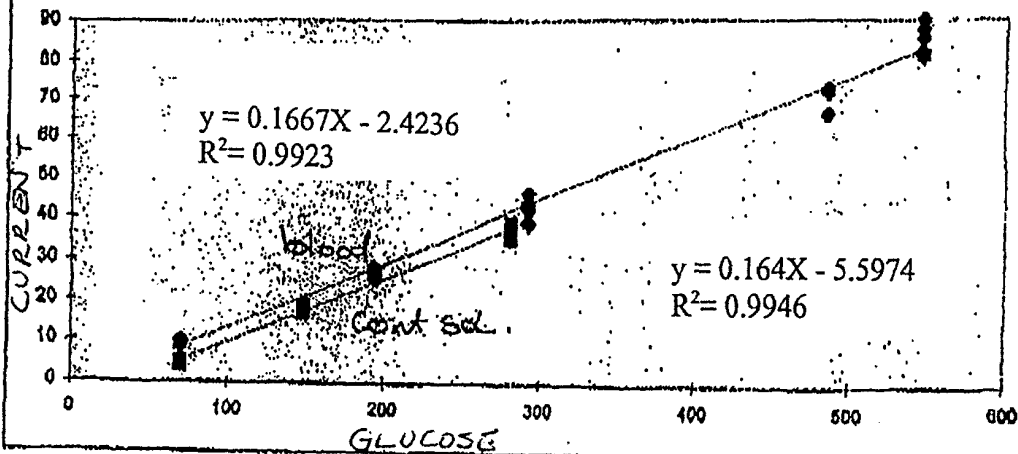


Fig. 6A

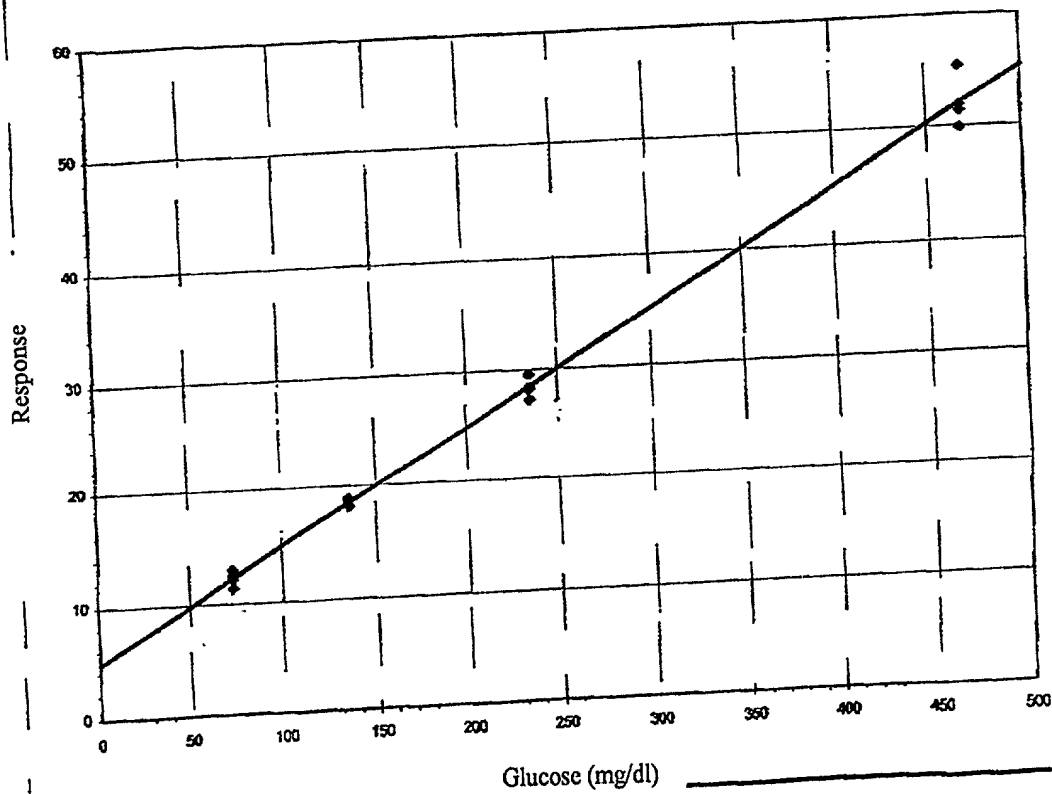


Fig. 6B

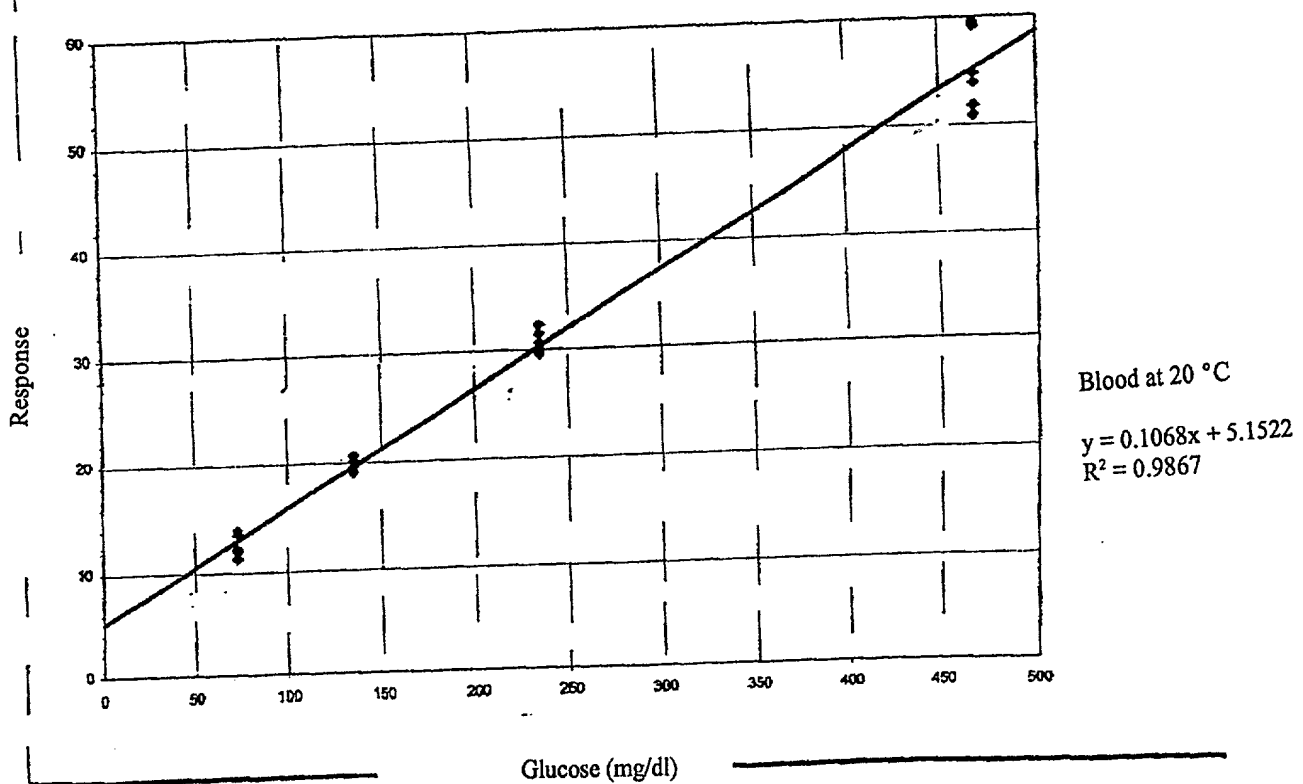


Fig. 7

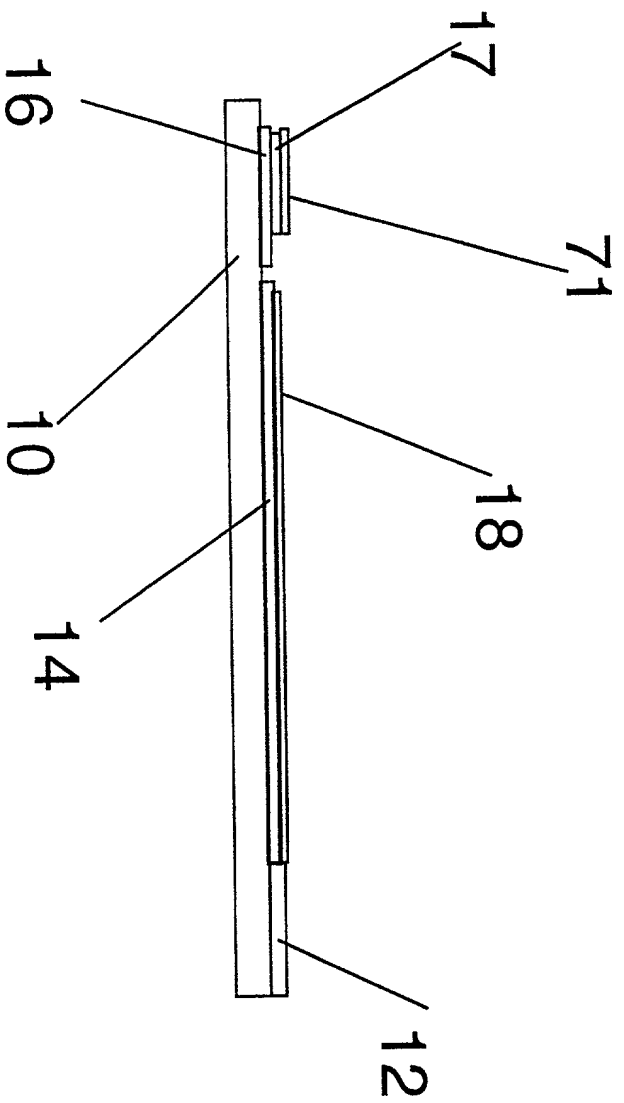


Fig 8A

**Silica Based Electrode**


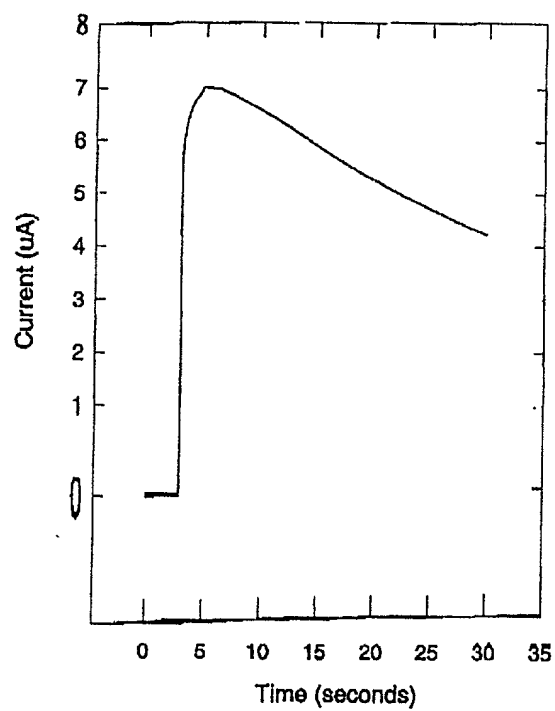


Fig 8B

**Carbon Based Electrode**

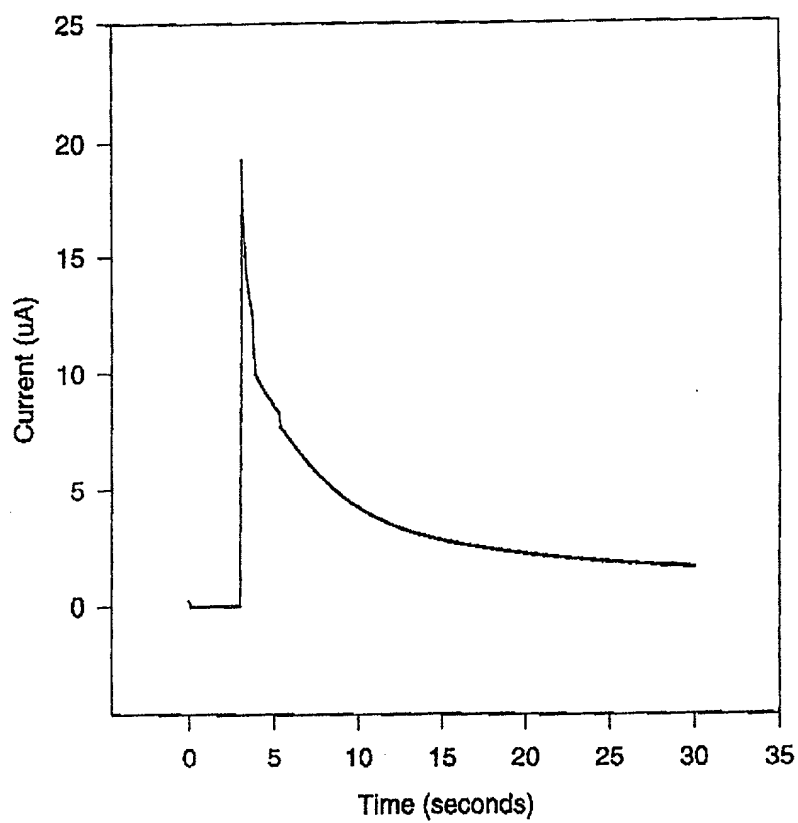

OPPEDAHL &amp; LARSON

FILE NO. SELF-P-005-US**COMBINED DECLARATION  
AND POWER OF ATTORNEY**

As a below named inventor, I hereby declare that:

My citizenship, residence and post office address are as listed below next to my name.

I believe I am the original, first and ☐ sole/☒ joint inventor of the subject matter which is claimed and for which a patent is sought on the invention entitled: DISPOSABLE GLUCOSE TEST STRIPS AND METHODS AND COMPOSITIONS FOR MAKING SAME  
the specification of which

(a) ☐ is attached hereto.

(b) ☒ was filed on February 14, 1996 as Application Serial No. 08/601,223 and was amended on \_\_\_\_\_.

(c) ☐ was described and claimed in International Application No. \_\_\_\_\_ filed on \_\_\_\_\_ and amended on \_\_\_\_\_.

**Acknowledgement of Duty of Disclosure**

I hereby state that I have reviewed and understood the content of the above identified specification, including the claims, as amended by any amendment referred to above. I acknowledge the duty to disclose information which is material to the patentability of the subject matter claimed in this application in accordance with Title 37, Code of Federal Regulations § 1.56(a).

**Continuation-In-Part Application**

I hereby claim the benefit under Title 35, United States Code, § 120 of any United States application(s) listed below and, insofar as the subject matter of each of the claims of this application is not disclosed in the prior United States application in the manner provided by the first paragraph of Title 35, United States Code § 112, I acknowledge the duty to disclose material information as defined in Title 37, Code of Federal regulations, § 1.56(a) which occurred between the filing date of the prior application and the national or PCT international filing date of this application:

(Application Serial No.) (Filing Date) (Status)(patented,pending,abandoned)

(Application Serial No.) (Filing Date) (Status)(patented,pending,abandoned)

**Power of Attorney**

I hereby appoint Carl Oppedahl, PTO Reg. NO. 32,746 and Marina T. Larson, PTO Reg. No. 32,038 of the firm of OPPEDAHL & LARSON, having office at 1992 Commerce Street, Yorktown Heights, NY 10598 as attorneys to prosecute this application and to transact all business in the Patent and Trademark Office connected therewith.

SEND CORRESPONDENCE TO:  
OPPEDAHL & LARSON  
1992 COMMERCE STREET, SUITE 309  
YORKTOWN HEIGHTS, NY 10598-4412

DIRECT TELEPHONE CALLS TO:  
OPPEDAHL & LARSON  
(914) 245-3252

OPPEDAHL & LARSON

FILE NO. SELF,P-005-US

**Claim for Priority**

I hereby claim priority under Title 35, United States Code, § 119 of any foreign application(s) for patent or inventor's certificate listed below and have identified any foreign applications for patent or inventor's certificate having a filing date before that of the application on which priority is claimed.

EARLIEST FOREIGN APPLICATION(S), FILED WITHIN TWELVE MONTHS (6 MONTHS FOR DESIGN) PRIOR TO SAID APPLICATION				
COUNTRY	APPLICATION NO.	DATE OF FILING (day/month/year)	DATE OF ISSUE (day/month/year)	PRIORITY CLAIMED
				YES <input type="checkbox"/> NO <input type="checkbox"/>
				YES <input type="checkbox"/> NO <input type="checkbox"/>
				YES <input type="checkbox"/> NO <input type="checkbox"/>

FOREIGN APPLICATION(S), IF ANY, FILED MORE THAN 12 MONTHS (6 MONTHS FOR DESIGN) PRIOR TO SAID APPLICATION				
COUNTRY	APPLICATION NO.	DATE OF FILING (day/month/year)	DATE OF ISSUE (day/month/year)	

I hereby declare that all statements made herein of my own knowledge are true and that all statements made on information and belief are believed to be true; and further that these statements are made with the knowledge that willful false statements and the like so made are punishable by fine or imprisonment or both, under Section 1001 of Title 18 of the United States Code and that such willful false statements may jeopardize the validity of the application or any patent issued thereon.

NAME OF SOLE OR FIRST INVENTOR	LAST NAME McAleer	FIRST NAME Jerome	MIDDLE NAME F.
RESIDENCE & CITIZENSHIP	CITY OF RESIDENCE	STATE OR COUNTRY OF RESIDENCE England	COUNTRY OF CITIZENSHIP United Kingdom
POST OFFICE ADDRESS 52 Notles Lane, GRWE		CITY WANTAGE	STATE/COUNTRY ZIP CODE OX12 0NR UK
DATE 1st July 1996		SIGNATURE JF McAleer	

- [x] Signature for additional joint inventor attached. Number of Pages 1.  
 [ ] Signature by Administrator(trix) or legal representative for deceased or incapacitated inventor. Number of Pages \_\_\_\_.  
 [ ] Signature for inventor who refuses to sign or cannot be reached by person authorized under 37 CFR § 1.47. Number of Pages \_\_\_\_.



FILE NO. SELF P-005-US

NAME OF SECOND INVENTOR	LAST NAME Scott	FIRST NAME David	MIDDLE NAME
RESIDENCE & CITIZENSHIP	CITY OF RESIDENCE	STATE OR COUNTRY OF RESIDENCE England	COUNTRY OF CITIZENSHIP
POST OFFICE ADDRESS 68 NEWLAND Mill		CITY WITNEY	STATE/COUNTRY ZIP CODE OXON OX8 6SZ
DATE 1st July 96		SIGNATURE D. Scott	
NAME OF THIRD INVENTOR	LAST NAME Hall	FIRST NAME Geoff	MIDDLE NAME
RESIDENCE & CITIZENSHIP	CITY OF RESIDENCE	STATE OR COUNTRY OF RESIDENCE	COUNTRY OF CITIZENSHIP
POST OFFICE ADDRESS WILLBOA DAMFIELD LANE		CITY INVERNESS	STATE/COUNTRY ZIP CODE IV2 3HS
DATE 1/7/96		SIGNATURE G. F. Hall	
NAME OF FOURTH INVENTOR	LAST NAME Icaza-Alvarez	FIRST NAME Manuel	MIDDLE NAME
RESIDENCE & CITIZENSHIP	CITY OF RESIDENCE	STATE OR COUNTRY OF RESIDENCE	COUNTRY OF CITIZENSHIP
POST OFFICE ADDRESS		CITY	STATE/COUNTRY ZIP CODE
DATE		SIGNATURE	
NAME OF FIFTH INVENTOR	LAST NAME Plotkin	FIRST NAME Elliott	MIDDLE NAME V.
RESIDENCE & CITIZENSHIP	CITY OF RESIDENCE	STATE OR COUNTRY OF RESIDENCE	COUNTRY OF CITIZENSHIP
POST OFFICE ADDRESS		CITY	STATE/COUNTRY ZIP CODE
DATE		SIGNATURE	

OPPEDAHL &amp; LARSON

FILE NO. SELF.P-005-US

NAME OF SECOND INVENTOR	LAST NAME Scott	FIRST NAME David	MIDDLE NAME
RESIDENCE & CITIZENSHIP	CITY OF RESIDENCE	STATE OR COUNTRY OF RESIDENCE England	COUNTRY OF CITIZENSHIP
POST OFFICE ADDRESS		CITY	STATE/COUNTRY ZIP CODE
DATE		SIGNATURE	

NAME OF THIRD INVENTOR	LAST NAME Hall	FIRST NAME Geoff	MIDDLE NAME
RESIDENCE & CITIZENSHIP	CITY OF RESIDENCE	STATE OR COUNTRY OF RESIDENCE	COUNTRY OF CITIZENSHIP
POST OFFICE ADDRESS		CITY	STATE/COUNTRY ZIP CODE
DATE		SIGNATURE	

NAME OF FOURTH INVENTOR	LAST NAME <i>Alvarez-Icaza</i> <del>Icaza-Alvarez</del>	FIRST NAME Manuel	MIDDLE NAME
RESIDENCE & CITIZENSHIP	CITY OF RESIDENCE	STATE OR COUNTRY OF RESIDENCE <i>United Kingdom</i>	COUNTRY OF CITIZENSHIP <i>Mexico</i>
POST OFFICE ADDRESS <i>3C Reay St</i>		CITY <i>Inverness</i>	STATE/COUNTRY ZIP CODE <i>IV2 3AJ</i>
DATE <i>1st July 1996</i>		SIGNATURE <i>[Signature]</i>	

NAME OF FIFTH INVENTOR	LAST NAME Plotkin	FIRST NAME <del>Elliott</del> ELLIOT	MIDDLE NAME V.
RESIDENCE & CITIZENSHIP	CITY OF RESIDENCE <i>INVERNESS</i>	STATE OR COUNTRY OF RESIDENCE <i>UNITED KINGDOM</i>	COUNTRY OF CITIZENSHIP <i>USA</i>
POST OFFICE ADDRESS <i>25 BROADSTONE PARK</i>		CITY <i>INVERNESS</i>	STATE/COUNTRY ZIP CODE <i>SCOTLAND, UK</i>
DATE <i>JULY 1 1996</i>		SIGNATURE <i>Elliott Plotkin</i>	